


PTCR ATH Temperature correction graph

Soaking time below the reference time of one hour causes a positive correction value, while soaking time above causes a negative value.

fired at different soak times under air and the atmospheric pressure

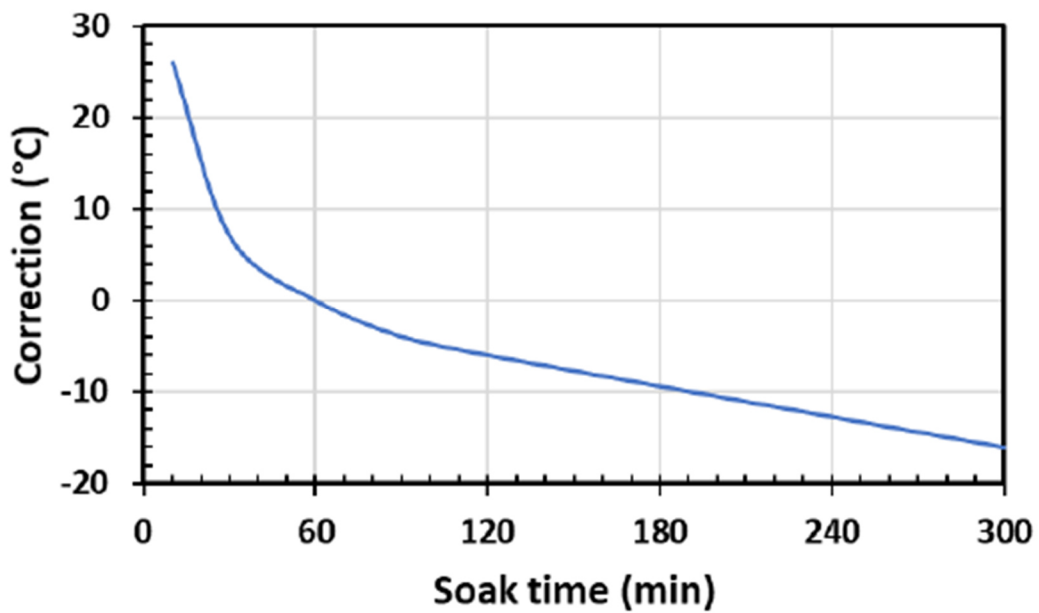

Soak time (min)	10	30	60	90	120	300
Correction (°C)	26	7	0	-4	-6	-16
Example	694	713	720	724	726	736