


PTCR UTH Temperature correction graph

Soaking time below the reference time of one hour causes a positive correction value, while soaking time above causes a negative value.

fired at different soak times under air and the atmospheric pressure

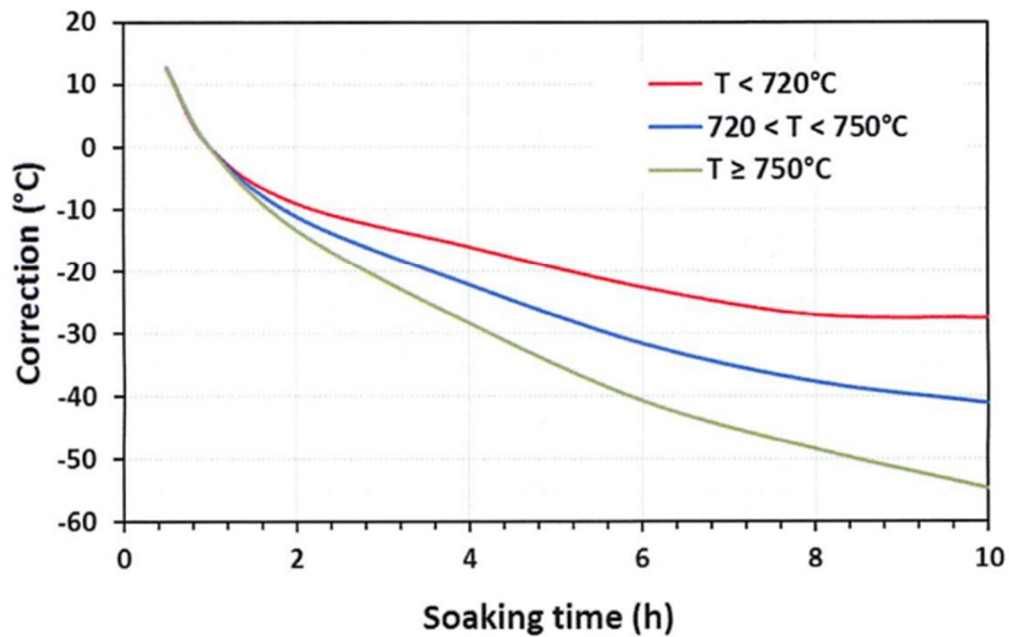

Soaking time (h)	0.5	1 (Ref.)	2	4	6	8	10
Correction (°C)	13	0	-13	-28	-41	-48	-55
Example	827	840	853	868	881	888	895